


WHICH ELECTRODE IS MOST APPROPRIATE?

The standard **StimRouter** electrode is appropriate for most patients and **StimRouter** implant locations. However, there are certain situations where **StimRouter** patients may benefit from a more specialized electrode design that better compliments patient anatomy and lead implant technique. Bioness is proud to offer the **StimRouter** Extended Electrode to help those patients enjoy the maximum relief that **StimRouter** can offer.

The **StimRouter** Extended Electrode may be considered for:

- Optimizing the stimulation circuit – remember the triangle
- Optimizing EPT orientation – new printed markings make patients' EPT placement easier than ever
- Optimizing stimulation of nerves in challenging anatomical locations
- Increased patient comfort while wearing the **StimRouter** electrode and EPT, depending on implant location.

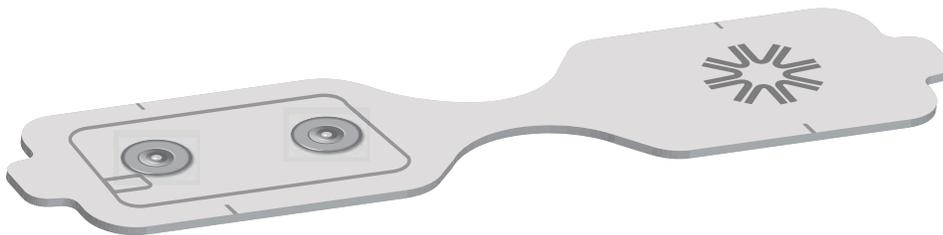


EXTENDED ELECTRODE




STANDARD ELECTRODE

ASK YOUR STIMROUTER REPRESENTATIVE WHICH ELECTRODE IS BEST FOR YOUR NEXT CASE!

EXTENDED ELECTRODE

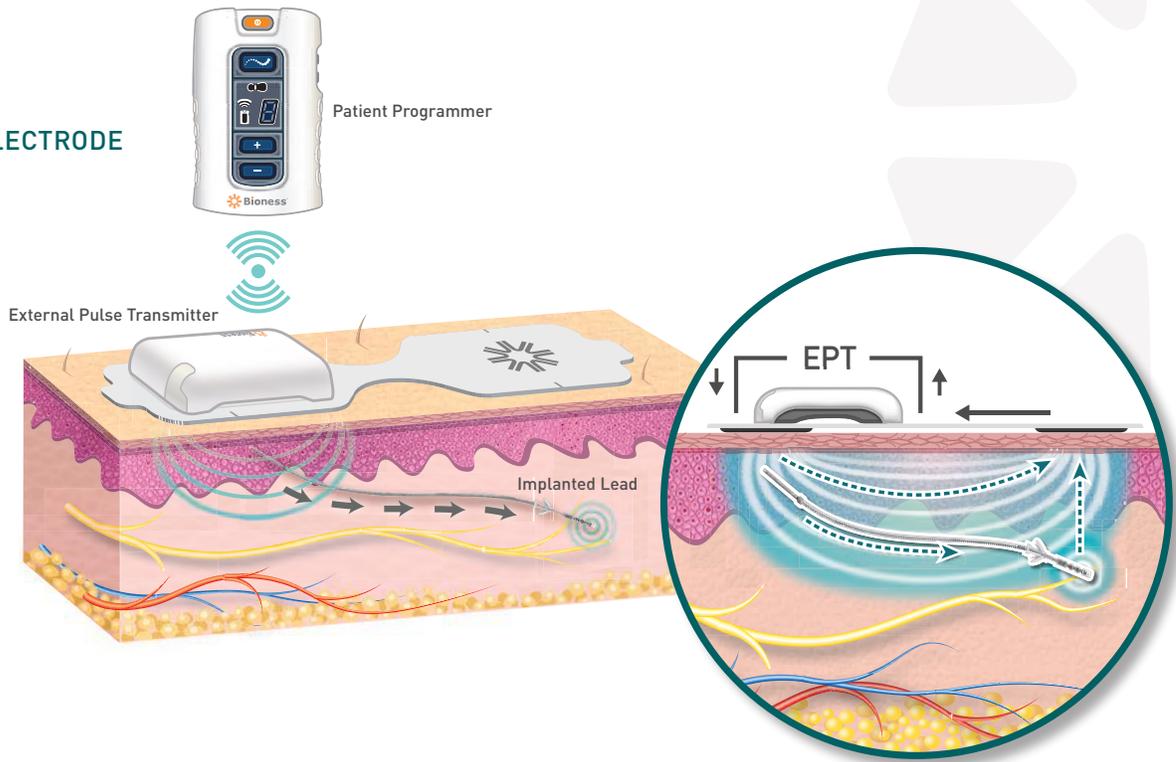

STANDARD ELECTRODE

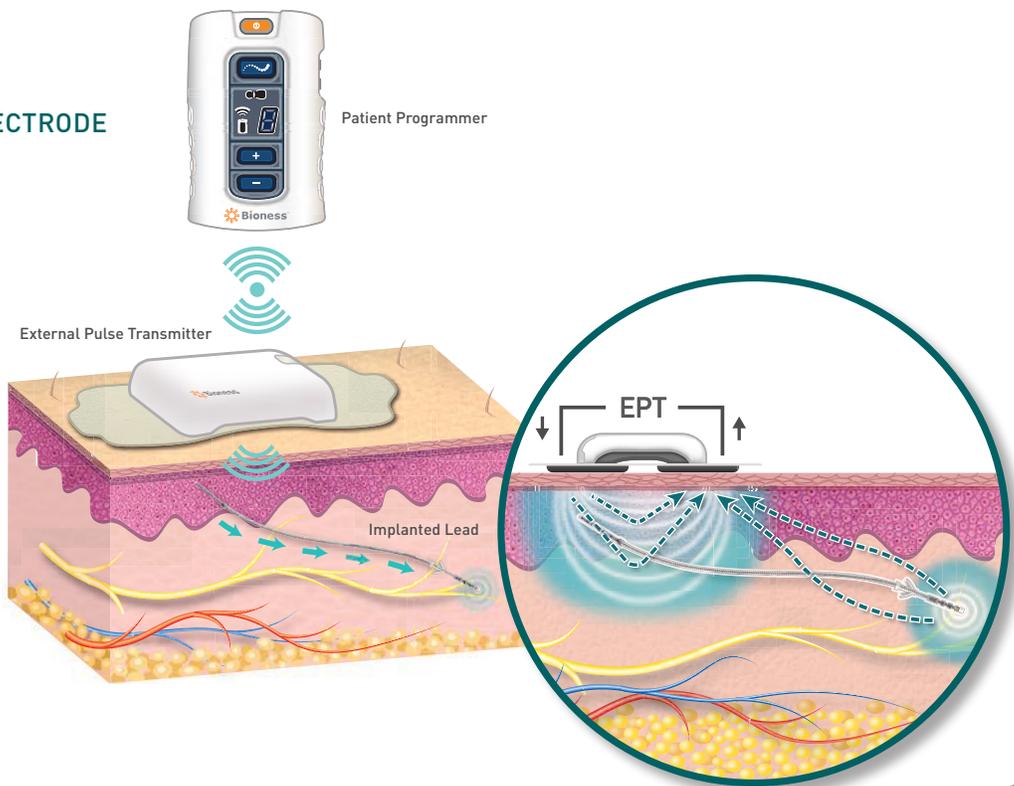

Individual results vary. Patients are advised to consult with a qualified physician to determine if this product is right for them.

Important Safety Information and Risks: For Indications for Use, Contraindications, Warnings, Adverse Reactions, Precautions and other safety information please refer to www.stimrouter.com/risks [also available in the StimRouter Clinician's Guide].

