


Which electrode is most appropriate?


The standard **StimRouter** electrode is appropriate for most patients and **StimRouter** implant locations. However, there are certain situations where **StimRouter** patients may benefit from a more specialized electrode design that better compliments patient anatomy and lead implant technique. Bioventus is proud to offer the **StimRouter** Extended Electrode to help those patients enjoy the maximum relief that **StimRouter** can offer.

The **StimRouter** Extended Electrode may be considered for:

- Optimizing the stimulation circuit
- Optimizing E-EFC orientation – new printed markings make patients' E-EFC placement easier than ever
- Optimizing stimulation of nerves in challenging anatomical locations
- Increased patient comfort while wearing the StimRouter electrode and E-EFC, depending on implant location.

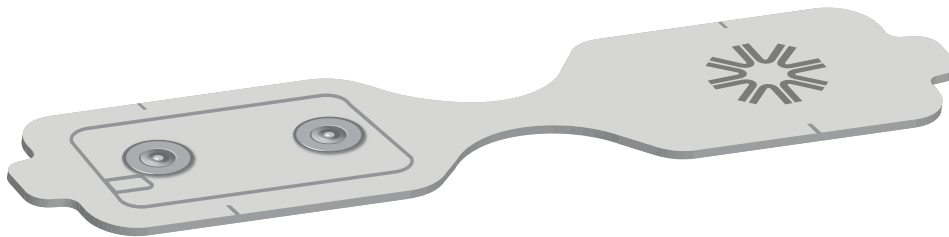


Extended Electrode

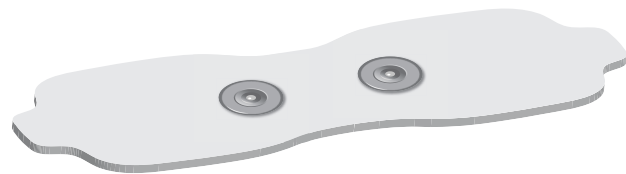


Standard Electrode

Ask your StimRouter Representative which electrode is best for your next case!

Extended Electrode

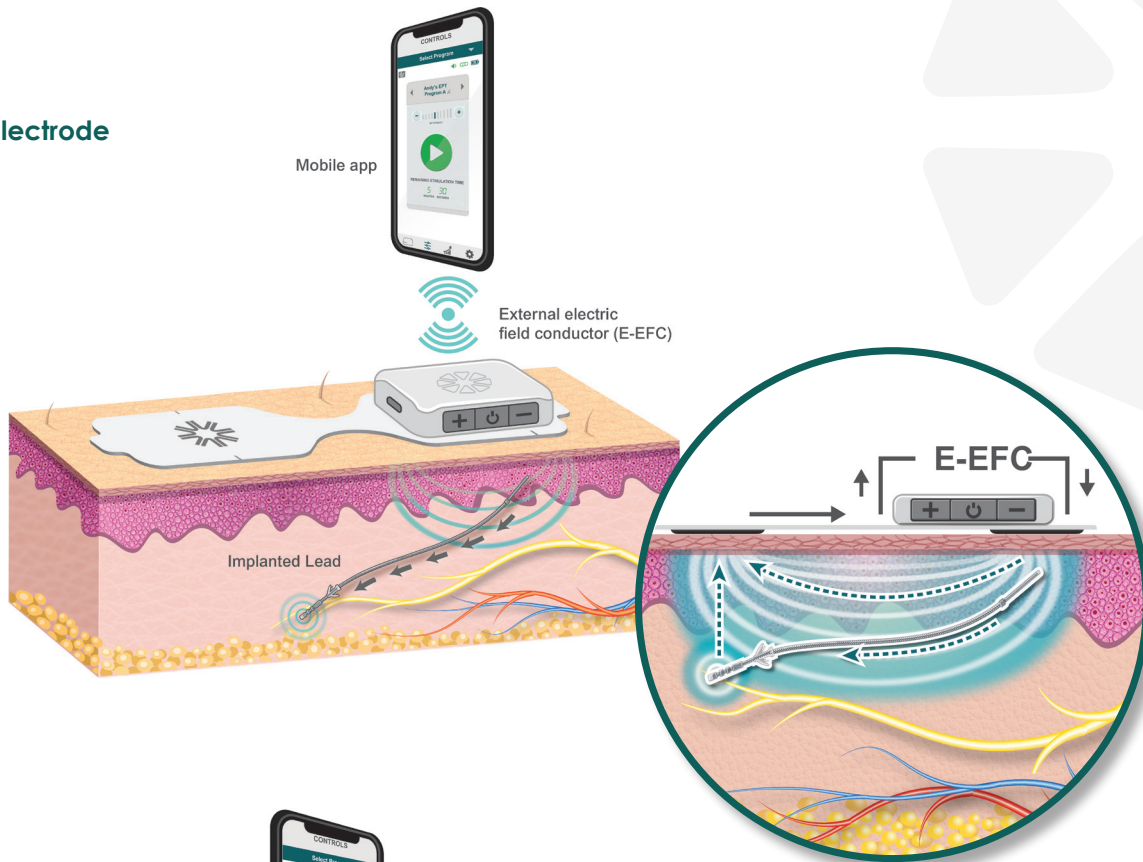

Standard Electrode

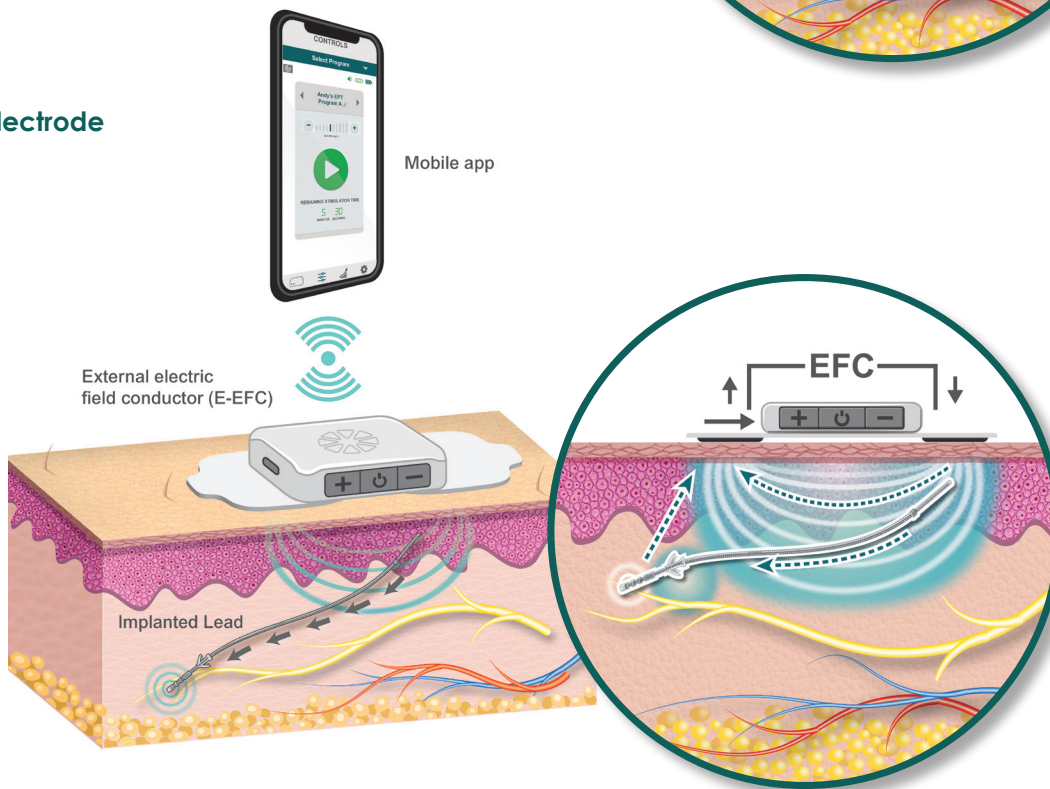

Indications for Use: The StimRouter Neuromodulation System is indicated for pain management in adults who have severe intractable chronic pain of peripheral nerve origin, as an adjunct to other modes of therapy (e.g., medications). The StimRouter is not intended to treat pain in the craniofacial region.

Do not use the StimRouter Neuromodulation System in users who have an implanted demand cardiac pacemaker, implanted cardioverter defibrillator (ICD), or other implanted active device, or who have bleeding disorders that cannot be stopped in advance of the StimRouter implantation procedure. Do not use the system where a metallic implant or a cancerous lesion is present in the immediate implant area. Effects of stimulation during pregnancy are not known. StimRouter is capable of producing skin irritation and muscle ache in the area of stimulation.

Full prescribing information can be found in the Clinician Guide or <https://stimrouter.com/safety-information>.

Bioventus and the Bioventus logo are registered trademarks of Bioventus LLC.
StimRouter is a registered trademark of Bioness Inc. | StimRouter.com | Rx Only

© 2024 Bioventus LLC SMK-004390A 07/24